

## SEMIAUTOMATIC AND FULLY FUNCTIONAL ELECTROCHEMICAL MICROANALYZER BO-05 SUITABLE FOR SCIENTIFIC, DIDACTIC AND ANALYTICAL APPLICATIONS: THE USE IN THE POTENTIOMETRIC ANALYSIS OF DRUGS

<sup>1</sup>Włodzimierz Opoka, <sup>1</sup>Marek Szłószarczyk, <sup>1</sup>Adam Chojnacki, <sup>1</sup>Agata Kryczyk-Poprawa\*, <sup>1</sup>Przemysław Talik, <sup>2</sup>József Gal, <sup>3</sup>Bożena Muszyńska, <sup>4</sup>Bogusław Baś

<sup>1</sup>Department of Inorganic and Analytical Chemistry, Pharmaceutical Faculty, Medical College, Jagiellonian University, 9 Medyczna St., 30-688 Kraków, Poland,

<sup>2</sup>Faculty of Engineering University of Szeged, Mars tér 7, 6724 Szeged, Hungary,

<sup>3</sup>Department of Pharmaceutical Botany, Pharmaceutical Faculty, Medical College, Jagiellonian University, 9 Medyczna St., 30-688 Kraków, Poland,

<sup>4</sup>AGH University of Science and Technology, Faculty of Materials Science and Ceramics, al. Mickiewicza 30, 30-059 Kraków, Poland,

e-mail: agata.kryczyk@uj.edu.pl

Received: February 11, 2021 • Accepted: February 24, 2021

### ABSTRACT

This article presents the potentiometric method of determination of chlorides using the original BO-05 electrochemical microanalyzer. The quantification of chlorides is one of the frequently performed methods, both in the indirect determination of active pharmaceutical ingredients (API) and impurities in pharmaceutical raw materials, pharmacopoeial substances or pharmaceutical formulations as well. Successfully validated method was used to the analysis of chlorides in the preparations containing verapamil hydrochloride in form of tablets Staveran<sup>®</sup> and Verapamil<sup>®</sup>. The mean content of the studied API calculated to one tablet was close to the declared and equal to 123.6±1.5 mg and 122.6±1.1 mg, respectively. The presence of excipients have no significant impact on the final results. Thus shown that the electrochemical microanalyzer BO-05 is suitable for scientific, didactic and analytical applications.

Keywords: potentiometric methods, potentiometric titration, electrochemical microanalyzer, verapamil hydrochloride

### 1. INTRODUCTION

The BO-05 microanalyzer combines both the functions of a potentiometer with high internal resistance and a potentiostat. The innovative BO-05 analyzer was constructed with the use of electronic devices and programmed appropriately for analytical purposes, using various types of sensors and microsensors, both scientific and educational. The analysis includes such methods as: potentiometry, stripping potentiometry, linear sweep voltammetry, anodic stripping voltammetry or chronoamperometry. The constructed microanalyzer is connected to a computer *via* the R-232 port which allows the manual and automatic control. Both the software and the equipment used minimize the amount of data necessary for the correct performance of the analysis and enabling quick online presentation of results. Direct connection with MS Office Excel enables immediate analysis of the obtained results and significantly improves the necessary calculations.

Verapamil (2-(3,4-dimethoxyphenyl)-5-[2-(3,4-dimethoxyphenyl)ethyl-methylamino]-2-propan-2-ylpentanenitrile;hydrochloride – Fig. 1) is currently one of the most widely used anti-arrhythmic drugs from the group of calcium channel blockers [1-4]. In pharmaceutical preparations, such as Staveran<sup>®</sup> and Verapamil<sup>®</sup>, it is used in doses of 40, 80 or 120 mg.

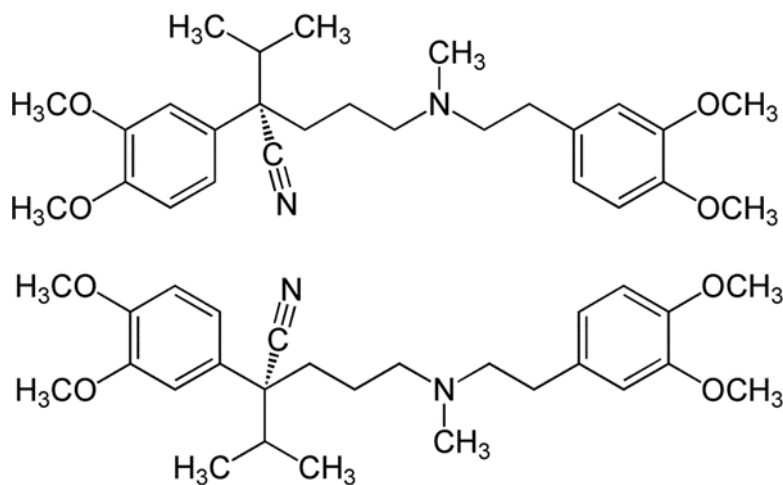


Figure 1. The chemical structure of verapamil

Verapamil is determined by various analytical techniques e.g. chromatographic [5-8], spectrophotometric [1], spectrofluorometric [9,10], voltamperometric [11], amperometric [12]. Verapamil with hydrochloride, in the studied pharmaceutical preparations, is present in a molar ratio of 1:1 [7]. Therefore, it is possible to determine the content of verapamil based on the amount of chlorides in this preparation. To determine the chloride content, a precipitometric method with a potentiometric end point detection was used. Standard solutions containing chlorides were titrated with silver nitrate(V) solution in the platinum electrode system as indicator and silver chloride electrode as reference. In this work, an attempt was made to indirectly determine the content of verapamil in the studied drugs, based on the analysis of the content of an equivalent amount of chlorides.


## 2. MATERIALS AND METHODS

### 2.1. Materials

Used in the research potassium nitrate ( $\text{KNO}_3$ ) and concentrated nitric acid ( $\text{HNO}_3$ ) were both Suprapur Merck. Water (quadruple-distilled) with a conductivity of less than  $1 \mu\text{S}/\text{cm}$  was obtained using an S2-97A2 distillation apparatus (ChemLand, Stargard Szczecin, Poland). The Staveran<sup>®</sup> (Medana Pharma SA) and Verapamil<sup>®</sup> (Mylan Pharmaceuticals Inc.) drugs were obtained in a local pharmacy.

## 2.2. Instrumentation

All potentiometric measurements were performed using a homemade BO-05 analyser (Fig. 2).

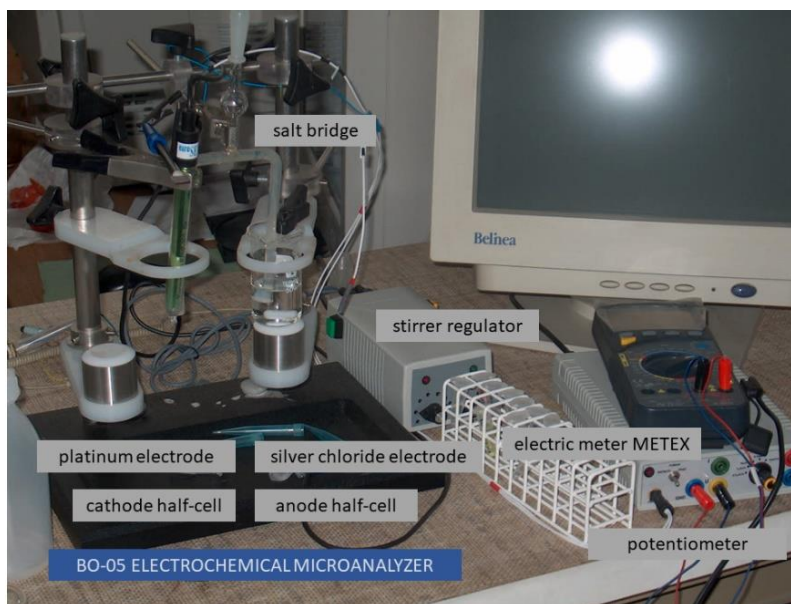

*Figure 2. The image of the Electrochemical Microanalyser BO-05*

The analyzer has been constructed using electronic components and programmed to be suitable for scientific, didactic and analytical applications using various electrochemical sensors and micro-sensors. The techniques accessible in the BO-05 analyzer include: various potentiometric methods, potentiometric stripping analysis, linear sweep voltammetry, anodic stripping voltammetry and chronoamperometry. The input impedance for potentiometer was greater than  $10^{15}$  ohms and the input current was lower than 0.1 pA. For driving potentiostat circuitry, potential range is  $\pm 8$  V, 2 mV potential resolution and 10 ms timing template are typical working parameters. The work of the analyzer is controlled manually and communicated with the computer by the RS-232 port. The applied hardware and software arrangement minimizes number of necessary data interchange transactions during measurement procedure and enables a true on-line presentation of measurement results.

The presented system for electrochemical analyses consists of three separate hardware modules: the analyzer BO-05, a desktop or mobile computer and electrodes stand.

The block diagram of BO-05 analyzer is shown on Fig. 3.



## 2.3. Methods

Before starting the analysis, 20 tablets of the each preparation under study were weighed and ground in a porcelain mortar. The obtained powder was partially accurately weighed and transferred quantitatively to a 50 mL volumetric flask and filled to the mark with quadruple-distilled water. The resulting solution was filtered.

5 mL of 1 M KNO<sub>3</sub> was added to the first of the measuring cell, and an appropriate amount of the sample solution, 20 µl of concentrated HNO<sub>3</sub> and quadruple-distilled water were added to the second one measuring cell. Half-cells were connected with each other using an electrolytic key filled with 10% agar gel and 0.1 M KNO<sub>3</sub>. 0.001 M AgNO<sub>3</sub> solution was added in equal portions to the measuring cell with the API under study at 10 s intervals. The SEM measurement of the measuring cell was recorded at 10 s intervals. Thus, 15 to 25 readings were obtained depending on the concentration of verapamil in the sample. The titration end point was determined automatically by the Hahn's method. The analyzes were performed in the Pt platinum electrode and Ag/AgCl silver chloride electrode.

The obtained results were developed with the use of a proprietary program Metex-bis, written in a Visual Basic. The statistical analysis was performed using the Statistica 10.0 program and the Microsoft Excel 2010 spreadsheet.

## 3. RESULTS

### 3.1. Method validation

#### 3.1.1. Precision

To check the precision of the method at one level, stock solution containing chlorides was prepared. Then, 100 µL of this solution with 50 µL of concentrated nitric acid were added into the measuring cell and filled with quadruple-distilled water up to 5 mL. The chlorides content in analyzed samples calculated to verapamil hydrochloride was 0.8 µg – Tab. 1. Fig. 4 shows examples of titration curves.

*Table 1. Results from method validation. Precision.*

No	sample [µg]	calculated amount [µg]	$\bar{x}$	SD	%RSD
1	0.800	0.827	0.810	0.021	2.59
2		0.843			
3		0.809			
4		0.779			
5		0.816			
6		0.816			
7		0.786			
8		0.793			
9		0.822			

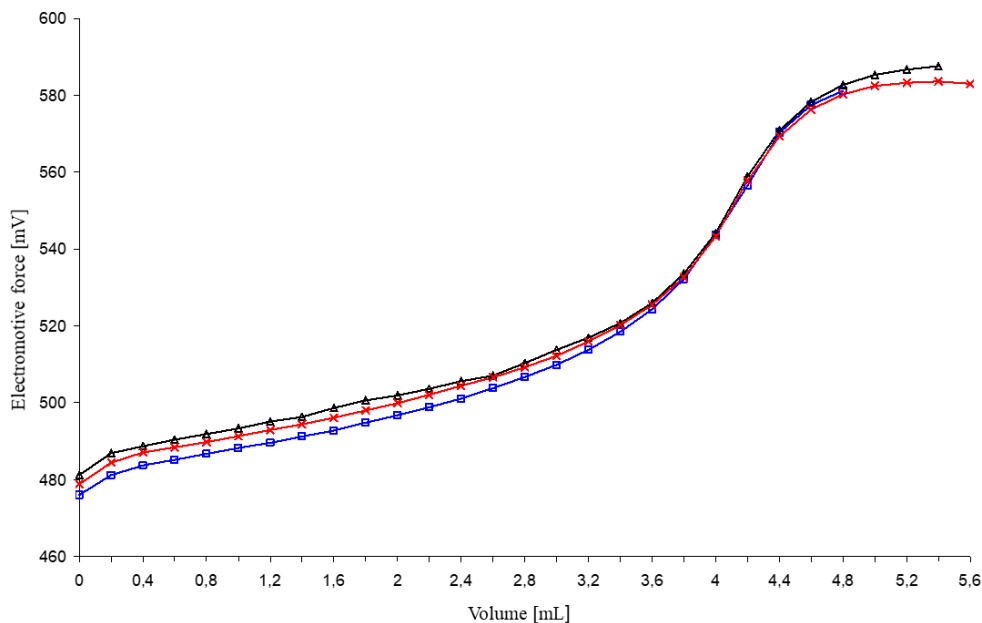


Figure 4. Examples of titration curves obtained for the same concentrations of standard chloride solutions

### 3.1.2. Linearity

To determine the linearity, 6 solutions at concentration in the range of 0.1 mmol/L - 1 mmol/L were prepared. The results were analyzed using the linear regression method. The regression equation and the correlation coefficient were as follows:  $y[V] = 0.1372 + 1.9857 \times c$ ;  $R = 0.9995$ .

### 3.1.3. Limit of detection and Limit of quantification

Using standard deviation and slope of a straight line coefficient. The values of LOD and LOQ were determined and equal to 0.1  $\mu\text{g}$  and 0.32  $\mu\text{g}$  respectively.

### 3.1.4. Specificity

Due to the similar properties of chlorides to iodides and bromides and the possibility of their presence next to each other. their influence on the end point of titration was investigated. The graph below shows the titration curves obtained for chlorides next to iodides and bromides. The method can be considered specific, because the PK values are clearly separable – Fig. 5.

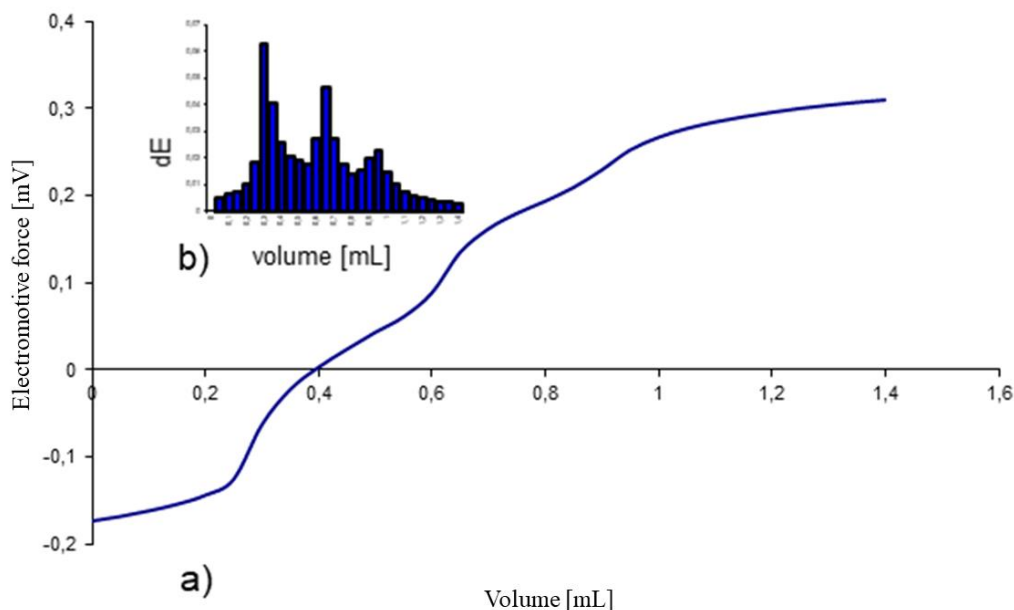


Figure 5. a) titration curve of chlorides in the presence of iodides and bromides; b) plot of the first derivative of the above determination

### 3.1.5. Accuracy

Recovery was calculated on the basis of determined content of verapamil hydrochloride to amount added to working solutions. The results are summarized in Tab. 2:

Table 2. The results of the recovery obtained for the Staveran® preparation and their statistical evaluation.

sample	% recovery	$\bar{x}$	SD	%RSD
1	99.65	99.78	1.98	1.98
2	99.63			
3	98.55			
4	103.68			
5	98.59			
6	98.60			

### 3.2. Analysis of pharmaceutical preparations

The pharmaceutical preparations of Verapamil® and Staveran® in the form of tablets were analyzed. The manufacturer's declared content of verapamil hydrochloride in each tablet is 120 mg. The obtained results of chlorides content in the weighted portion of prepared samples enabled to determine the content of verapamil in samples under study – Tab. 3. In the next step, the calculated amounts were converted into the average content of the active substance under study per 1 tablet of the pharmaceutical preparation of Verapamil® and Staveran® - Tab. 4.



Table 3. The content of verapamil hydrochloride determined in samples under study.

weighted portion [mg]	declared content [mg]	determined average amount [mg]	SD	%RSD	n
613.2	309.0	315.8	12.8	4.06	6
604.4	304.6	318.4	12.7	4.00	6
605.3	305.0	318.2	9.6	3.00	6
849.7	298.26	307.3	4.7	1.52	6
850.7	298.61	311.1	5.2	1.66	6
782.0	274.50	289.2	6.5	1.68	6

Table 4. Calculated content of verapamil hydrochloride in preparations per 1 tablet of the pharmaceutical preparation Verapamil® and Staveran®.

pharmaceutical preparation	average amount per 1 tablet [mg]	SD	%RSD	n
Staveran® 120 mg	123.6	1.46	1.1	6
Verapamil® 120 mg	122.6	1.08	0.88	6

## 4. CONCLUSIONS

Due to the obtained results, it can be concluded that the analytical method using the BO-05 microanalyzer is an effective and reliable in the indirect determination of verapamil in selected pharmaceutical preparations. Under conditions of experiment, the method featured high sensitivity, good precision and comparability of results as proven by the method validation and statistical analysis of the results. The presence of excipients in the formulation have no significant impact on the results. Due to the low cost and relatively short duration of the analysis as well as the significant automation. This method can be proposed as comparable to other methods of determining of drugs.

## REFERENCES

- [1] Al-Ghannam SM. 2006 A simple spectrophotometric method for the determination of  $\beta$ -blockers in dosage forms. *Journal of Pharmaceutical and Biomedical Analysis* 40(1). 151-156
- [2] Liu J.-F. 2011 The impact of verapamil on catecholamine polymorphic ventricular tachycardia. *Acta Cardiologica Sinica* 27(2). 115-119
- [3] Brogden RN. Benfield P. 1996 Verapamil: a review of its pharmacological properties and therapeutic use in coronary artery disease. *Drugs*. 51(5). 792-819. doi: 10.2165/00003495-199651050-00007.
- [4] Singh BN. Ellrodt G. Peter CT. 1978 Verapamil: a review of its pharmacological properties and therapeutic use. *Drugs*. 15(3). 169-97. doi: 10.2165/00003495-197815030-00001.
- [5] Pourkarim F. Rahimpour E. Jouyban A. 2019 Analytical techniques for the determination of verapamil in biological samples and dosage forms: An overview. *Bioanalysis* 11(23). 2189-2205
- [6] Pourkarim F. Shayanfar A. Khoubnasabjafari M. et al. 2019 Determination of verapamil in exhaled breath condensate by using microextraction and liquid chromatography. *Current Pharmaceutical Analysis* 15(5). 535-541.
- [7] Vijayabaskar S. Mahalingam V. Kalaivani. 2017 Analytical method development and validation for the analysis of verapamil hydrochloride and its related substances by using ultra performance liquid chromatography. *Journal of Pharmaceutical and Biomedical Analysis* 137. 189-195.



- [8] Jhee OH. Hong JW. Om AS. Lee MH. Lee WS. Shaw LM. Lee JW. Kang JS. 2005 Direct determination of verapamil in rat plasma by coupled column microbore-HPLC method. *Journal of Pharmaceutical and Biomedical Analysis* 37 (2). 405-410.
- [9] Walash M. Belal F. El-Enany N. Abdelsalam A. 2006 Spectrofluorometric determination of verapamil hydrochloride in pharmaceutical preparations and human plasma using organized media: Application to stability studies. *Journal of AOAC International* 89 (6). 1565-1572.
- [10] Walash MI. Belal F. El-Enany N. Abdelal AA. 2009 Kinetic Spectrofluorometric Determination of Certain Calcium Channel Blockers via Oxidation with Cerium (IV) in Pharmaceutical Preparations. *International Journal of Biomedical Science* 5(2). 146–157.
- [11] Kasim EA. Ghandour MA. El-Haty MT. Ahmed MM. 2003 Determination of verapamil by adsorptive stripping voltammetry in urine and pharmaceutical formulations. *Journal of Pharmaceutical and Biomedical Analysis* 30 (4). 921-929.
- [12] Ortuño JA. Sánchez-Pedreño C. Gil A. 2005 Flow-injection pulse amperometric detection based on ion transfer across a water-plasticized polymeric membrane interface for the determination of verapamil. *Analytica Chimica Acta* 554 (1-2). 172-176.